


easySpiral Dilute[®]

The world's first automatic diluter & plater

A revolution
in serial dilutions!

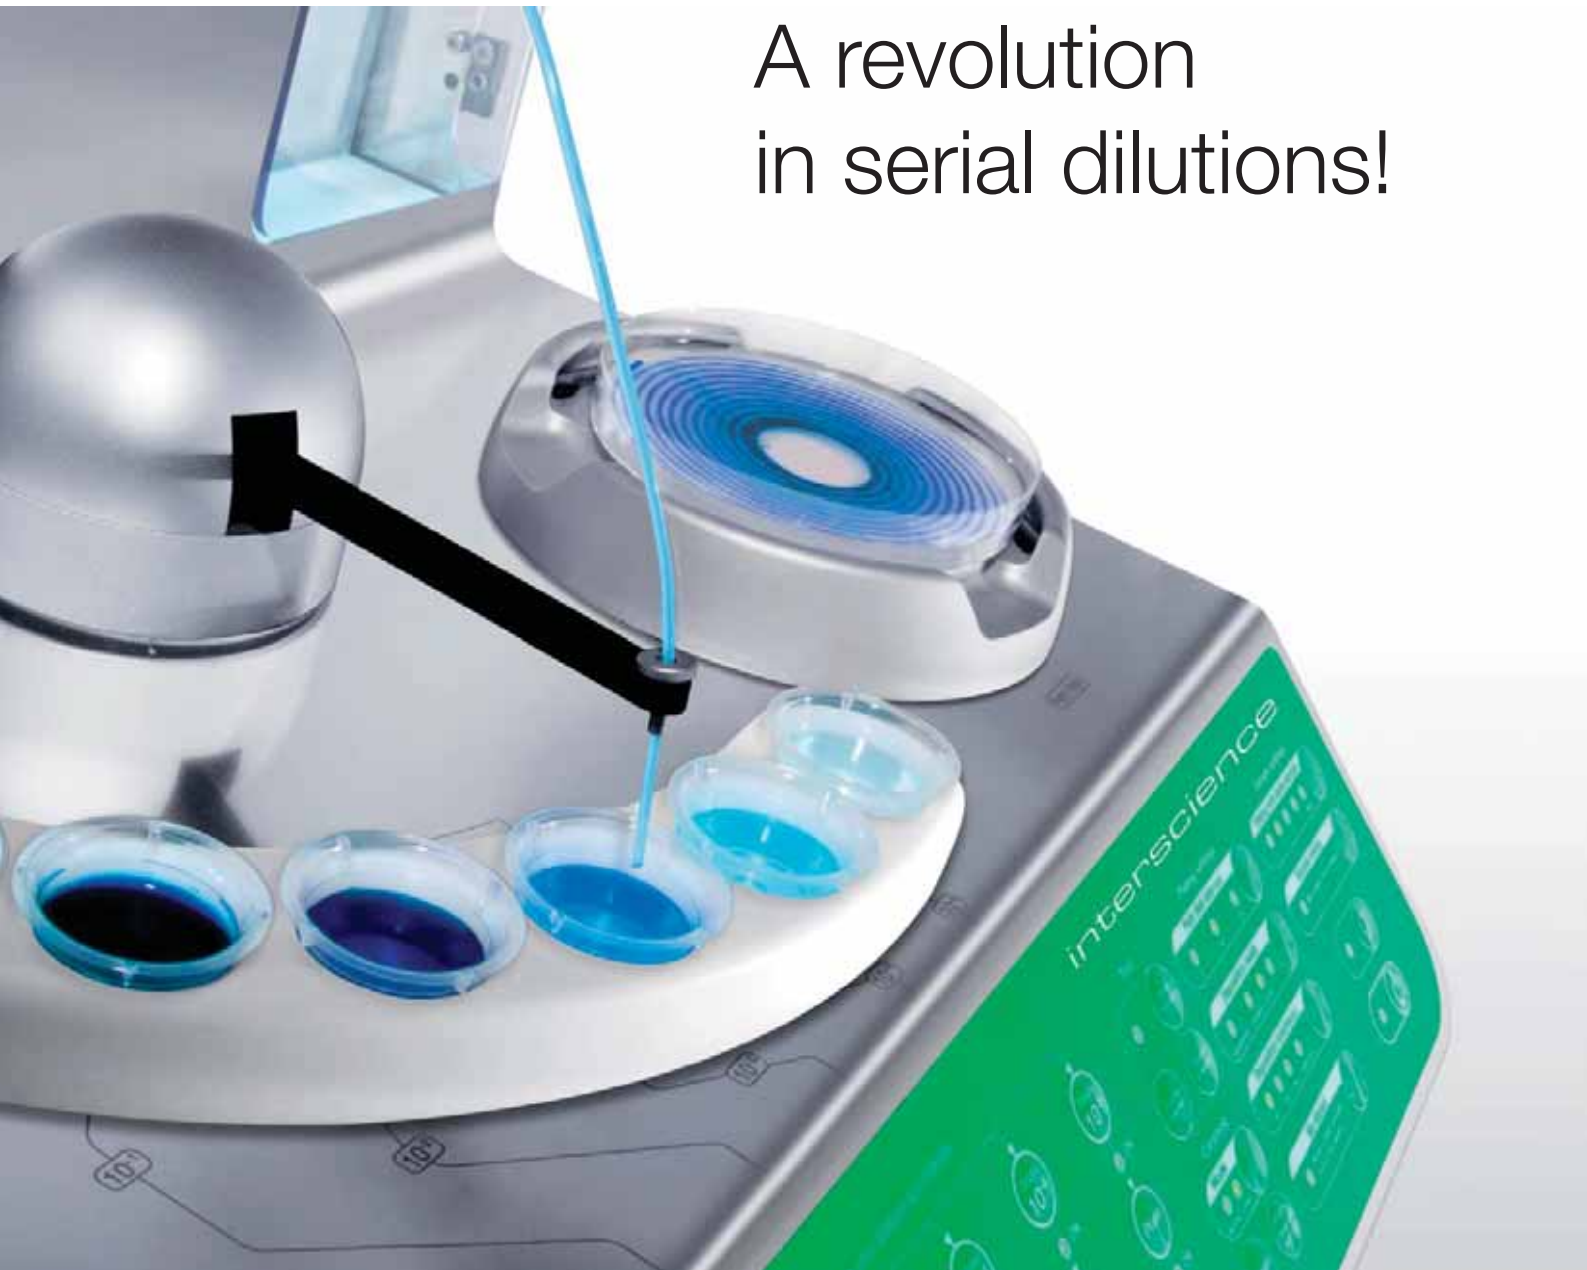

interscience

interscience

Our quality for your lab

- Designer and manufacturer for microbiology
- R&D leadership for innovative and reliable products
- Worldwide distribution network in more than 90 countries
- Made in France



interscience
R&D center and manufacturing plant
Mourjou FRANCE

Spiral[®] method: 35 years experience


The Spiral[®] method was designed in 1973 to automate the routine work of bacterial enumeration by Dr. Ed Campbell, researcher at the FDA (Food & Drug Administration). With François Jalenques, friend and founder of interscience, they patented an updated method in 1992.

Since then Spiral[®] automatic platers have been a reference for applications in food microbiology, medical bacteriology, research on food preservatives or cosmetological factors in compliance with the NF V08-050, NF V08-034, ISO 7218, ISO 4833-2, ISO 15189, FDA BAM and AOAC 977.27 standards.

Today interscience is proud to launch the 4th generation of Spiral[®] platers with easySpiral Dilute[®]: the world's first automatic diluter & plater.




F. Jalenques & Dr. Ed Campbell

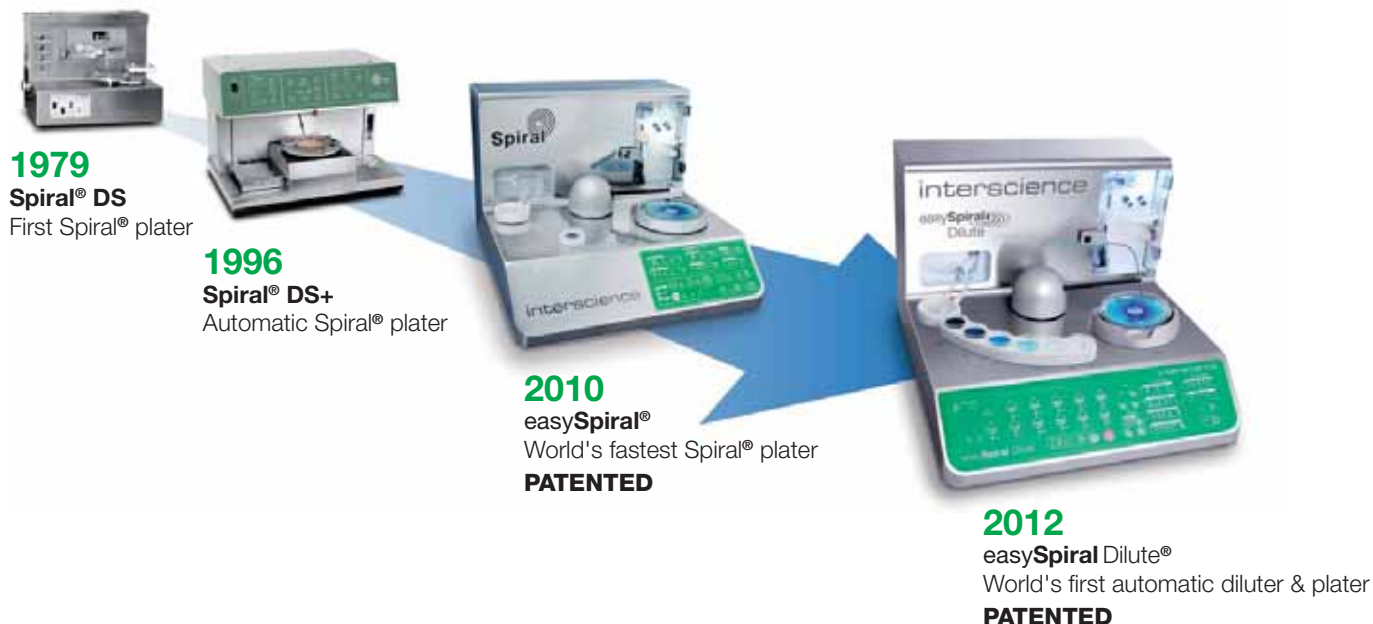

interscience is proud to introduce easySpiral Dilute®, a **2-in-1 automatic diluter and plater**, which allows you to do **5 x 1/10th serial dilutions**. It will then automatically plate on 1 single Petri dish, with a countable range from **30 to 1 x 10¹² countable CFU/mL**.

No more manual dilutions and plating is automatic!

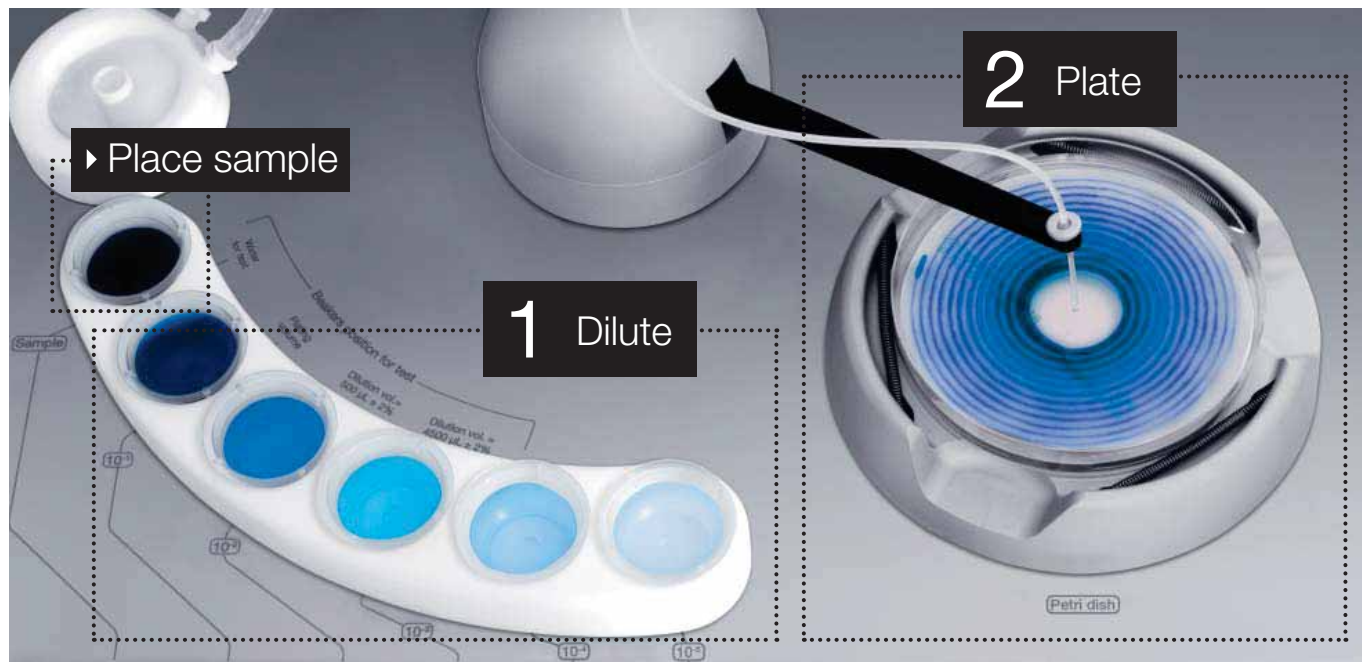

- ▶ Place your sample in the beaker
- 1. The easySpiral Dilute® will automatically dilute the sample up to 5 times
- 2. The easySpiral Dilute® will automatically plate the sample on a Petri dish up to 1 x 10¹² countable CFU/mL

Why use an automatic diluter & plater?

easySpiral Dilute® allows you to **save 50% on consumables and 50% on your time**.

Comparison between manual and automatic method below.

Example of 50 samples: Dilution: 10⁻⁷
Plating: 10⁻⁵, 10⁻⁶ and 10⁻⁷

⊖ Manual method

CONSUMABLES

Dilution

- 400 tubes
- 350 pipet tips

Plating

- 450 Petri dishes

TIME 10h10

⊕ Automatic method

CONSUMABLES

Dilution

- 350 beakers

Plating

- 150 Petri dishes

TIME 5h50

Key features

Compact

40 cm wide, can be used inside and outside a laminar flow
Stainless steel housing

High precision

Glass syringe typical accuracy of 0.5 %
No more pipet calibration

High speed automation

Fast rotating arm
1 disinfection, 5 dilutions and 1 plating in 134 s
PATENTED



Automatic disinfection

Overflow technology cleaning system
No cross contamination
PATENTED

One-touch plating

Choose from 4 plating modes
Plate on 55, 90 and 150 mm Petri dishes

Easy serial dilutions


Choose your dilution factor
Do 10^{-5} dilution or more automatically
No more 9 mL tube preparation
PATENTED

Cleaning autonomy


2 fully autoclavable bottles
(disinfectant & diluent) and connectors

How does it work?

1. Dilution cycle

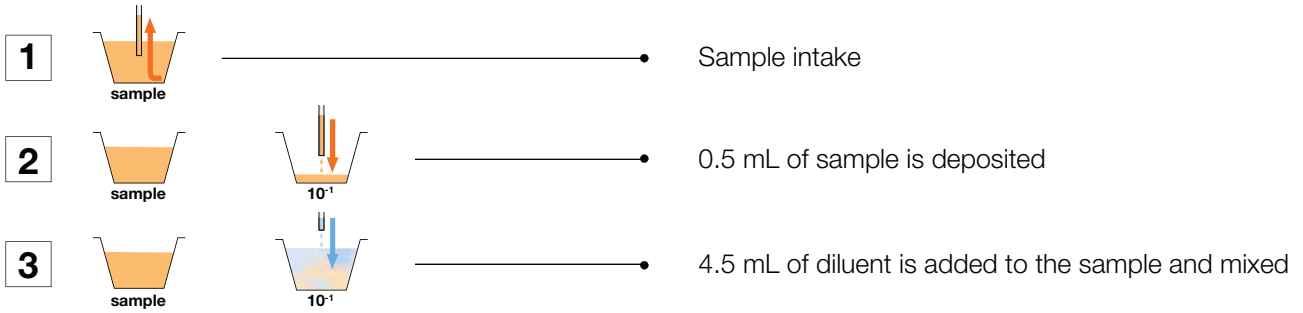

The above dilution cycle is repeated for the next serial dilution.

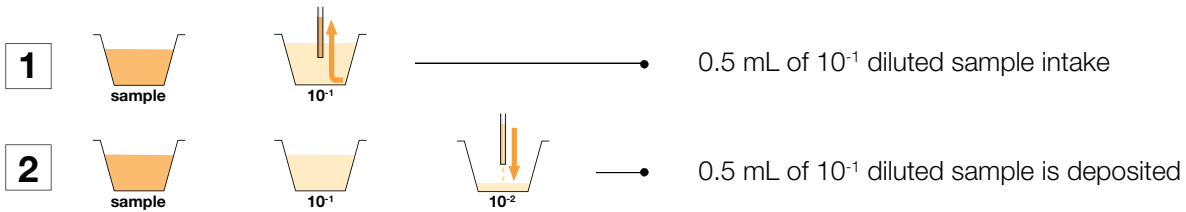

Dilution cycle can be repeated as many times as you wish.


2. Plating cycle

	Constant mode	Exponential mode	Circle mode	Pour mode
	Homogenous surface deposition 50 μ L, 100 μ L, 200 μ L and USB programmable	Decreasing surface concentration 50 μ L, 100 μ L, 200 μ L and USB programmable	3 or 6 surface dilutions on 1 Petri dish 10 μ L inner circle, 16 μ L middle circle and 25 μ L outer circle	Homogenous deposition* in pour plate mode 50 μ L, 100 μ L, 200 μ L and USB programmable
Examples:				

* In pour mode, easySpiral Dilute® deposits one sample drop at the bottom of an empty Petri dish. Then, the user adds the molten agar on top and homogenizes it with the sample.

How to count?

Manual colony counting

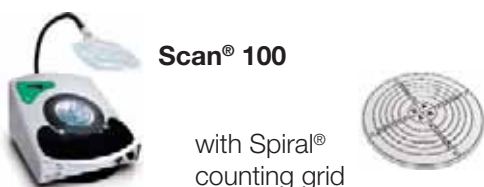


or

Automatic colony counting



Questions

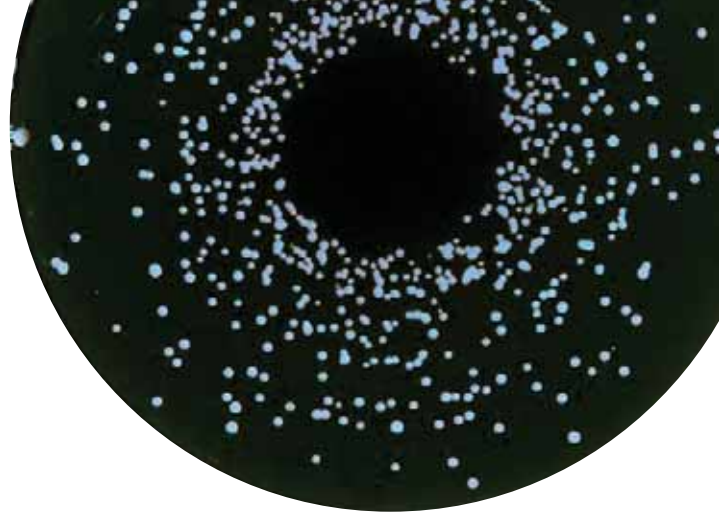

What is special about the easySpiral Dilute®?

easySpiral Dilute® is the only 2-in-1 equipment on the market making automatic serial dilutions and standardized plating.

The accuracy of easySpiral Dilute® is high: 0.5%. How can I check it?

It is easy and automatic.

Test of the deposited volume during plating:
Press on the plating volume test button. This function will fill a previously weighed beaker with 500 µL. Weigh the distributed volume to check the results.

Test of the volume of the dilutions:
Press on the dilution volumes test button. This function will fill 2 previously weighed beakers: one with 0.5 mL and the 2nd one with 4.5 mL. Weigh the distributed volumes to check the results.

I usually dilute 1 mL to 1/10 and the easySpiral Dilute® uses 0.5 mL to 1/10. Is easySpiral Dilute® as precise with a volume divided by 2?

Usually the average accuracy for the 9 mL tubes filling and 1 mL pipetting is 2% with the need to calibrate and regularly check the pipets you are using.

easySpiral Dilute® has an average accuracy of 0.5% on 0.5 mL and 4.5 mL volumes because it works with a high precision Hamilton™ glass syringe in a liquid displacement circuit.

With volumes divided by 2, precision and repeatability are then much higher!

Which diluents can I use?

easySpiral Dilute® works with saline solutions (e.g.: Ringer's solution, physiological saline).

Avoid using diluents with nutrients as they may cause contaminations. Bacteria only remain a few seconds in the beakers before being deposited on the Petri dish so using a saline diluent has no effect on the final enumeration.

It is however possible to use nutrient solutions as diluent in the semi-automatic "My Diluent" mode. In that case, fill in the beakers with 4.5 mL diluent before processing.

I need to make a 10⁻⁷ dilution. How can I do it?

The easySpiral Dilute® can do as many dilutions as you wish.

Do a 10⁻⁵ dilution, take the last beaker and place it as the mother sample and then proceed with a new automatic dilution sequence.

Accessories & technical specifications



Housing protection

Transparent housing for working outside laminar flow.

Ref. 413 001

dataLink™

Traceability system

Ref. 410 100

DB50 Beakers

1 000 sterile beakers for Spiral® platers (5 mL)

Ref. 415 100


Barcode reader

Barcode reader for traceability

Ref. 522 000

easySpiral Dilute® is delivered with 1 000 DB50 beakers, 1 blue dye for tests, 1 EnzyClear® liquid detergent, 1 syringe, 2 filters, 1 stylus, 4 connection kit for GL 45 bottle, 1 double connection kit for GL 45 bottle, Petri dish rings: 55, 90 & 150 mm, Spiral® counting grids: 90 & 150 mm, circle counting grids: 90 & 150 mm, power cord, user's manual, monitoring CD-ROM software, USB cable.

Reference	easySpiral Dilute®
	414 000
Petri dish diameter	55 mm, 90 mm and 150 mm
Syringe capacity	1 000 µL
Programmable dispensed volume (via USB)	from 10 µL to 1 000 µL
Preset dispensed volume	50 µL, 100 µL and 200 µL
Counting range	from 30 to 1x10 ¹² CFU/mL
Plating modes	55 mm: constant, pour plate 90 mm: exponential (10 ⁻⁵), constant, circle (3 dilutions), pour plate 150 mm: exponential (10 ⁻⁷), constant, circle (6 dilutions), pour plate
Number of dilutions at 1/10 th for 1 cycle	5
1 disinfection + 5 dilutions + 1 plating of 1 dilution	134 s
1 disinfection + 5 dilutions + 1 plating of each dilution	234 s
Disinfectant autonomy	1000 (with 2 L bottles)
Diluent autonomy	63 cycles (with 2 L bottles)
Circle mode (patented)	3 dilutions on a 90 mm Petri dish 6 dilutions on a 150 mm Petri dish
Stylus disinfection system (patented)	inside and outside by Overflow technology
Pressure in the stylus	jusqu'à 8 bars
Successive plating capacity with the same sample	up to 20 Petri dishes (50 µL)
Traceability	excel™, datamatrix labels
Disinfection process	✓
Filling time and volume programmable via USB	✓
My Diluent key	✓
Sample mixing before dilution/plating	✓
Controlled by microprocessor	✓
Dimensions (w x d x h)	40 x 41.5 x 29 cm
Weight	16.4 kg
Power supply	100-240 V~ / 50 Hz to 60 Hz
Power	65 W
1 year guarantee (after registration)	✓
All stainless steel	✓
Made in France	✓





interscience

30, ch. Bois Arpents - 78860 St Nom - FRANCE
T: +33 (0)1 34 62 62 61 - F: +33 (0)1 34 62 43 03
Email: info@interscience.com

interscience USA & CANADA

32 Cummings Park - Woburn, MA 01801 - USA
T: +1 781 937 0007 - F: +1 781 937 0017
Email: sales.usa@interscience.com

interscience CHINA

上海市徐汇区吴兴路277号锦都大厦588室-200030
电话: +86 (0)21-64739390 - +86 189 3097 0733
邮址: sales.china@interscience.com

interscience SOUTH-EAST ASIA

541 Orchard Rd - 09-01 Liat Towers - SINGAPORE 238881
T: +65 6933 1389 - +65 8549 1217
Email: sales.asia@interscience.com

Your local distributor



IGZ Instruments AG
Furtbachstrasse 17
8107 Buchs ZH

Tel. +41 44 456 33 33
igz.ch igz@igz.ch